PLEASE CAREFULLY READ THE INSTRUCTIONS BEFORE YOU START. Use these instructions in conjunction with your antigen test kit or PCR test instructions.

RHINOMED

RHINOSWAB JUNIOR SAMPLE UCTIONS R USE

TO BE USED UNDER THE GUIDANCE OF AN ADULT.


Go into the nostrils Break Line Novelty Handle RHINOSWAB JUNIOR by RHINOMED®

Loops

HANDLE, remove the swab YOUR HANDS. out of its packaging.

2: TOUCHING ONLY THE


Do not use if pouch is damaged





1: WASH OR SANITIZE


5: SET TIMER FOR 30 SECONDS and ask the child to breathe normally through their nose.





Set timer for **30 SECS**

PLEASE TURN OVER

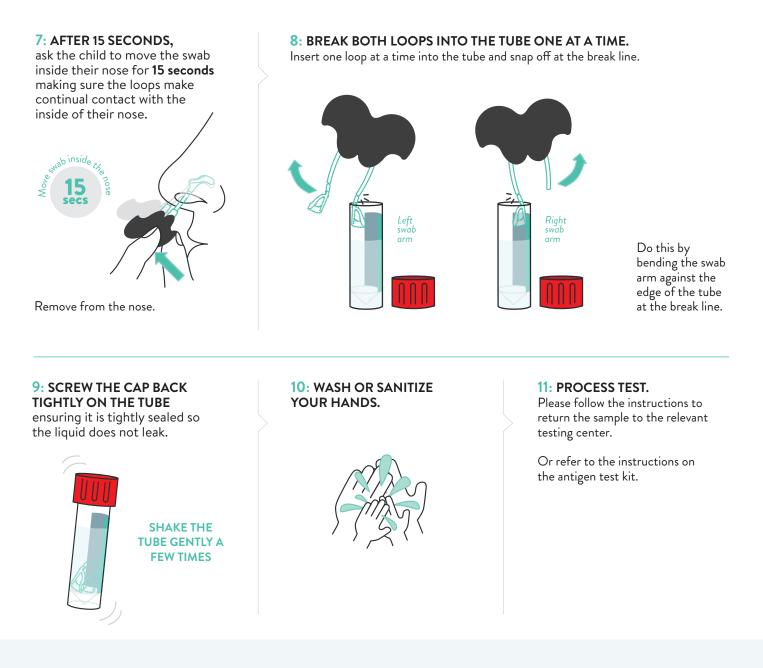

| SYMBOL | MEANING | SYM |
|-----------------------------|--|------|
| | RHINO MED Level 1, 132 Gwynne St, Cremorne VIC 3121 swab@rhinoswab.global | |
| MD Patent Pending | Medical device | |
| (2) | Do not reuse | U |
| 2 | Temp 2-30 degree | L |
| * | Exposure to sunlight | R |
| \Box | Use before | STER |

| SYMBOL | MEANING |
|-----------|---|
| ĺ | Consult the instructions for use |
| | Do not use if packaging is damaged |
| UDI | Unique device identifier |
| LOT | Individual lot number |
| REF | Manufacturer catalogue/reference number |
| sterile r | Gamma radiation |

Rhinomed Ltd Level 1, 132 Gwynne St, Cremorne VIC 3121 swab@rhinoswab.global RMS-904 | REVB | 2 March 2023